


SEAL THORACIC STENT GRAFT

Inward Bending
Delayed Deployment System
Sufficient Radial Force
Complete Sealing zone
Excellent Flexibility & Conformability
4,6,8,10mm Tapered



CASE



Case1

Pre CT 3D image

Post CT 3D image




Case2

Pre CT 3D image

Post CT 3D image

Comparison Chart

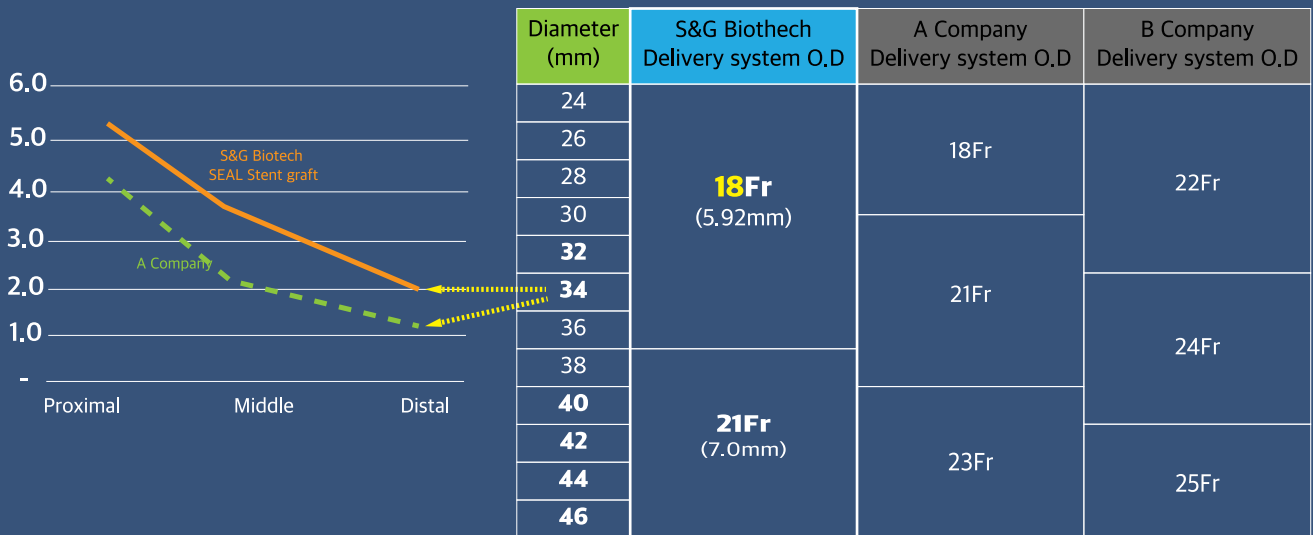

Ordering Information

Type	Ordering No.	Size			
		Diameter (mm)	Length (mm)	Delivery System	
				Diameter OD(ID)Fr	Usable Length(cm)
Thoracic Limb Stent	Limb-**-** Limb-**-***	22	60 ~ 200	15 (13)	90
		24 ~ 36		18 (16)	
		38 ~ 46		21 (19)	

Ordering Information (Ordering No. 1st **: Diameter(mm) / Last **: Length(mm))

Type	Ordering No.	Diameter (mm)		Length (mm)	Delivery System	
		Proximal Diameter(mm)	Distal Diameter(mm)		Diameter OD(ID)Fr	Usable Length(cm)
26	20,22					
28	20,22,24					
30	20,22,24,26					
32	22,24,26,28					
34	24,26,28,30	80, 110, 130, 150, 180, 200				
36	26,28,30,32					
38	28,30,32,34					
40	30,32,34,36					
42	32,34,36,38					
44	34,36,38,40	80, 110, 130, 150, 180, 200	21 (19)			
46	36,38,40,42					

Ordering Information (Ordering No. 1st **: Proximal Diameter(mm) / 2nd **: Distal Diameter(mm) / 3rd **: Length(mm))



S&G BIOTECH INC.
E-Mail. sng@sngbio.co.kr

82, Bugok-ro, Pogok-eup, Cheoin-gu, Yongin-si, Gyeonggi-do, Korea (PO) 17023
Tel. +82 31.748.6625 Fax. +82 31.748.6620